




EC Series Instruction Manual

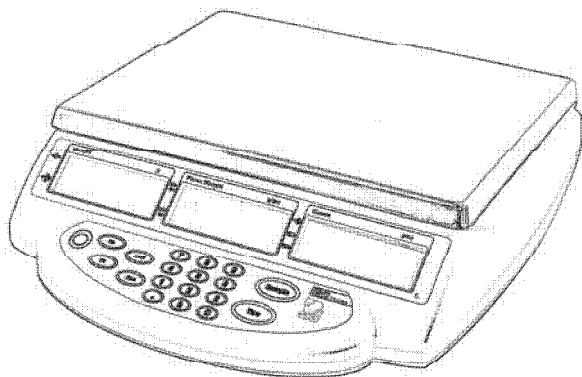

Ohaus Corporation, 19A Chapin Road, PO Box 2033, Pine Brook, NJ 07058 USA

Declaration of Conformity We, Ohaus Corporation, declare under our sole responsibility, that the scale models listed below are in conformity with the directives and standards mentioned.


Declaración de Conformidad Nosotros, Ohaus Corporation, declaramos bajo responsabilidad exclusiva que los modelos de básculas indicados a continuación están conformes con las directivas y normas citadas.

Déclaration de conformité Nous, Ohaus Corporation, déclarons sous notre seule responsabilité, que les types de balances ci-dessous cités sont conformes aux directives et aux normes mentionnées ci-après.

Konformitätserklärung Wir, die Ohaus Corporation, erklären in alleiniger Verantwortung, dass die untenstehenden Waagentypen mit den genannten Richtlinien und Normen übereinstimmen.

Dichiarazione di conformità Noi, Ohaus Corporation, dichiariamo sotto nostra unica responsabilità, che i tipi di bilance specificati di seguito sono conformi alle direttive e norme citate.

Models/Type / Modelo/Tipo / Modèle/Type / Modell/Typ / Modello/Tipo: **EC3, EC6, EC15, EC30**

EC Marking: Marcado EC Marquage CE EC-Markierung Marcature EC	EC Directive Directiva EC Directive CE EC Richtlinie Direttiva EC	Applicable Standards Normas aplicables Normes applicables Geltende Standards Standard applicabili
	73/23/EEC Low Voltage Baja tensión Basse tension Niederspannung Bassa tensione	EN61010-1:2002
	89/336/EEC Electromagnetic compatibility Compatibilidad electromagnética Compatibilité électromagnétique Elektromagnetische Verträglichkeit Compatibilità elettromagnetica	EN61326:2002

Date: October 1, 2004



Ted Xia
President
Ohaus Corporation
Pine Brook, NJ USA



Urs Müller
General Manager
Ohaus Europe
Greifensee, Switzerland

Note: This equipment has been tested and found to comply with the limits for a Class A digital device, pursuant to Part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference when the equipment is operated in a commercial environment. This equipment generates, uses, and can radiate radio frequency energy and, if not installed and used in accordance with the instruction manual, may cause harmful interference to radio communications. Operation of this equipment in a residential area is likely to cause harmful interference in which case the user will be required to correct the interference at his own expense.

This Class A digital apparatus complies with Canadian ICES-003.

Cet appareil numérique de la classe A est conforme à la norme NMB-003 du Canada.

ISO 9001 Registration

In 1994, Ohaus Corporation, USA, was awarded a certificate of registration to ISO 9001 by Bureau Veritus Quality International (BVQI), confirming that the Ohaus quality management system is compliant with the ISO 9001 standard's requirements. On May 15, 2003, Ohaus Corporation, USA, was re-registered to the ISO 9001:2000 standard.

Registro ISO 9001

En 1994, Bureau Veritus Quality International (BVQI) le otorgó a Ohaus Corporation, EE.UU., un certificado de registro ISO 9001 el cual confirma que el sistema administrativo de calidad de Ohaus cumple con los requerimientos del estándar ISO 9001. En mayo 15 del 2003, Ohaus Corporation, EE.UU., fue registrada nuevamente al estándar ISO 9001:2000.

Enregistrement ISO 9001

En 1994, le Bureau Veritus Quality International (BVQI) a octroyé la certification d'enregistrement ISO 9001 à Ohaus Corporation, États-Unis d'Amérique, confirmant que le système de gestion de la qualité Ohaus était conforme aux conditions normalisées de l'ISO 9001. Le 15 mai 2003, Ohaus Corporation, États-Unis d'Amérique, a été ré-enregistrée à la norme ISO 9001:2000.

Registrierung nach ISO 9001

Im Jahr 1994 wurde der Ohaus Corporation, USA, ein Zertifikat der Registrierung nach ISO 9001 vom Bureau Veritus Quality International (BVQI) verliehen, in dem bestätigt wird, dass das Ohaus-Qualitätsmanagementsystem den Anforderungen der Norm ISO 9001 entspricht. Am 15. Mai 2003 wurde die Ohaus Corporation, USA, gemäß der Norm ISO 9001:2000 neu registriert.

Registrazione ISO 9001

Nel 1994, Ohaus Corporation, USA, ha ricevuto il certificato di registrazione ISO 9001 da Bureau Veritus Quality International (BVQI), come conferma che il sistema di gestione della qualità Ohaus risponde alle caratteristiche standard di ISO 9001. Il 15 Maggio 2003, Ohaus Corporation, USA, è stata riregistrata per la normativa ISO 9001:2000.

1 INTRODUCTION	EN-2
1.1 Product Description	EN-2
1.2 General Features	EN-2
1.3 Safety Precautions	EN-2
2 INSTALLATION	EN-3
2.1 Unpacking	EN-3
2.2 Installing Components	EN-3
2.3 Selecting the Location	EN-3
2.4 Leveling the Scale	EN-3
2.5 Connecting Power	EN-4
2.6 Initial Calibration	EN-4
3 OVERVIEW OF CONTROLS AND FUNCTIONS	EN-5
3.1 Display Symbols	EN-5
3.2 Controls and Functions	EN-6
4 OPERATIONS	EN-7
4.1 Switching the Unit On and Off	EN-7
4.2 Manual Tare	EN-7
4.3 Pre-set Tare	EN-7
4.4 Zero Operation	EN-8
4.5 Sampling, Calculating Average Piece Weight (APW)	EN-8
4.6 Entering a Known Piece Weight	EN-8
4.7 Storing Piece Weight into Memory	EN-9
4.8 Recalling Piece Weight from Memory	EN-9
4.9 Accumulation: Weight and Quantity	EN-9
5 SCALE SETTINGS	EN-10
5.1 Auto-Off	EN-10
5.2 Zero Tracking Range	EN-10
5.3 Zero Display Range	EN-10
5.4 Filtering	EN-10
5.5 Zero Return Range	EN-11
5.6 Backlight	EN-11
5.7 Unit Selection	EN-11
5.7 APW Re-computing	EN-11
6 CALIBRATION	EN-12
7 TROUBLESHOOTING	EN-12
8 TECHNICAL DATA	EN-13

1 INTRODUCTION

This manual contains installation, operation and maintenance instructions for the EC Series counting scale. Please read the manual completely before installation and operation.

1.1 Product Description

The EC Series is an economical compact counting scale designed for fast, accurate operation ideally suited for annual inventories, parts rooms, rentals and other counting applications. Combining an internal accuracy of 1:600,000, Average Piece Weight (APW) of 0.01g/0.00002lb to 0.1g/0.0002lb (depending on model) and an internal rechargeable battery, the Ohaus EC Series scale offers accuracy, durability and portability in one easy-to-use design.

1.2 General Features

- ☑ Capacity models: 3000g/6lb, 6000g/15lb, 15000g/30lb, 30000g/60lb with maximum displayed resolution of 1:30,000.
- ☑ Stainless steel weighing pan
- ☑ Durable plastic housing with protective cover
- ☑ 3-window, backlit LCD with prominent 19mm high digits
- ☑ Fast display of Weight, Average Piece Weight (APW) and Parts Count.
- ☑ Gram or pound weighing units
- ☑ Low sample weight and APW indication
- ☑ Full counting keypad with numeric keys
- ☑ Dedicated TARE and SAMPLE keys for simple and fast operation
- ☑ Accumulator function for weight and parts count
- ☑ Adjustable filtering level for weighing under various conditions
- ☑ Auto-optimization recalculates APW constantly for enhanced counting accuracy
- ☑ 10-APW memory locations
- ☑ 80-hour Internal rechargeable battery with power-saving Auto-shut off feature

1.3 Safety Precautions



For safe and dependable operation of this scale, please comply with the following safety precautions:

- ☑ Verify that the input voltage printed on the AC Adapter and the plug type matches the local AC power supply.
- ☑ Make sure that the power cord does not pose a potential obstacle or tripping hazard.
- ☑ Disconnect the scale from the power supply when cleaning the scale.
- ☑ Do not operate the scale in hazardous or unstable environments.
- ☑ Do not immerse the scale in water or other liquids
- ☑ Do not drop loads on the platform.
- ☑ Use only approved accessories and peripherals, as available.
- ☑ Operate the scale only under ambient conditions specified in these instructions.
- ☑ Service should be performed by authorized personnel only.

2 INSTALLATION

2.1 Unpacking

Unpack and verify that the following components have been included:

- ☑ EC Scale
- ☑ Weighing Platform (plastic base with stainless steel pan)
- ☑ Instruction Manual
- ☑ AC Adapter


Save the packaging material. This packaging ensures the best possible protection for the storage or transport of the product.

2.2 Installing Components

Position the weighing platform pins into the through-holes on the top housing, then set the platform securely into place.

IMPORTANT:

- ☑ **BEFORE USING THE SCALE, REMOVE THE SHIPPING PROTECTION SCREW** located underneath the scale. This screw ensures protection of the load cell during transport, but will need to be removed for the scale to operate properly.




- ☑ It is recommended that the protective screw be re-installed if transporting the scale. Do not over-tighten the protective screw as it may damage the load cell. To re-install, turn the scale on and place a 500g weight on the pan, then slowly screw in the protection screw until the display shows a value between 250g to 400g.

2.3 Selecting the Location

Operate the scale on a firm, level surface. Avoid locations with rapid temperature changes, excessive dust, moisture, air currents, vibrations, electromagnetic fields, heat or direct sunlight.

2.4 Leveling the Scale

Adjust the leveling feet until the bubble is centered in the circle of the level indicator (located on the front panel).



NOTE: Ensure that the scale is level each time its location is changed.

2.5 Connecting Power


2.5.1 AC Power

Verify that the intended AC power source matches the AC adapter rating. Connect the supplied AC adapter to the power input receptacle underneath the scale. Plug the AC adapter into a properly grounded power outlet.

2.5.2 Battery Power

The battery will begin charging with the AC adapter connected accordingly. An LED indicator below and to the right of the Count window shows the status of battery charging:

- Green – battery is fully charged
- Yellow – battery is partially charged and charging
- Red – battery is nearly discharged

When AC power is not available, the scale will operate on the internal rechargeable battery. The scale will automatically switch to battery operation if there is a power failure or the power cord is removed. Low battery charge is indicated by the  annunciator (the scale will operate for approximately 10 hours more before automatically switching off).

Before using the scale for the first time, the internal rechargeable battery should be fully charged for up to 12 hours. A fully charged battery can operate the scale for approximately 80 hours independent of AC power. The scale can be operated during the charging process. The battery is protected against overcharging and the scale can remain connected to the AC power line.

NOTES:

- ☑ The battery must be recharged every 3 months if the scale is not used for a long time.
- ☑ Dispose of the lead acid battery according to local laws and regulations



CAUTION

**BATTERY IS TO BE REPLACED ONLY BY AN AUTHORIZED OHAUS SERVICE DEALER.
RISK OF EXPLOSION CAN OCCUR IF REPLACED WITH THE WRONG TYPE OR
CONNECTED IMPROPERLY**


2.6 Initial Calibration

When the scale is operated for the first time, a Span Calibration is recommended to ensure accurate weighing results. Before performing the calibration, be sure to have the appropriate calibration weights.

Refer to *Section 6* for Span Calibration procedures.

3 OVERVIEW OF CONTROLS AND FUNCTIONS

3.1 Display Symbols

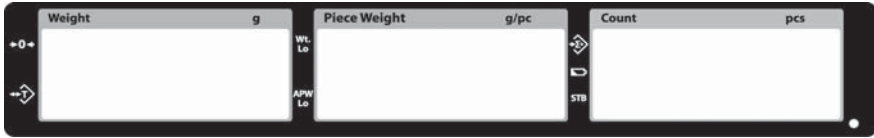

“WEIGHT”



“PIECE WEIGHT”

“Wt. Lo”

“APW Lo”

“COUNT”



“STB”

o LED

- Weight Window - displays weight of object on weighing pan, or accumulated weight value
- Center of Zero Indication
- Tare or Pre-set Tare (PT) Indication
- Piece Weight Window - displays the Average Piece Weight (APW) value, or number of weighments
- Low Sample Weight Indication - total sample weight is less than 10 display divisions, add more samples for more accurate reading
- Low Average Piece Weight Indication - calculated APW is less than 1/10 display divisions, unit weight is too small for ensuring accurate quantity calculations
- Piece Count Window - displays the calculated number of pieces on the weighing pan, or accumulated piece count value
- Scale is in Accumulation mode
- Low battery charge, recharge battery
- Stable Indication, scale is in stable condition
- Battery Charging Indication:
 - o Green – battery is fully charged
 - o Yellow – battery is partially charged and charging
 - o Red – battery is nearly discharged

3.2 Controls and Functions



Sample

- Inputs the indicated sample size and weight to calculate APW



Tare

- Inputs the weight of the object on the weighing pan as a Tare value
- Long press – enters user setup mode



APW

- Inputs the indicated unit weight value entered via the numeric keypad



Zero

- Zeros the display
- Long press – initiates calibration



PT

- Inputs the indicated value entered via the numeric keypad as a Pre-set Tare value



M+

- Adds the indicated weight or piece count value into Accumulation memory
- Long press - recalls and displays the total Accumulation data: weight, count and number of weighments



C

- Clears the indicated input values

0-9-.

- 11 x Numeric keys, 0-9 and decimal point

4 OPERATIONS

4.1 Switching the Unit On and Off

The power switch is located underneath the right-hand side of the scale. Push the switch to the "I" position to turn the scale on, and to the "O" position to turn the scale off. Allow 15-30 minutes for the scale to warm up before use.

NOTE: Make sure the weighing pan is empty before turning the scale on.

4.2 Manual Tare

Tare is indicated by the \leftrightarrow T annunciator.

Place the container on the weighing pan (ex. 100g), then press **TARE**. "TARE" will be displayed momentarily before the weight is tared.

Weight g	Piece Weight g/pc	Count pcs
100.0	0.	0.
-----	TARE	-----
0.0	0.0	0.

4.3 Pre-set Tare

Pre-set Tare is a known tare value entered via the numeric keypad

Pre-set Tare is indicated by the \leftrightarrow T annunciator.

With an empty pan:

Press **PT**, "PrEtA" will flash on the display. Enter a numeric value (ex. 200g), then press **PT**. The Pre-set Tare will be displayed as a negative value (no weight on the pan).

Weight g	Piece Weight g/pc	Count pcs
0.0	PrEtA	-----
200.0	PrEtA	-----
-200.0	0.	-----

With an existing weight on the pan (ex. 250g):

Press **PT**, "PrEtA" will flash on the display. Enter a numeric value (ex. 200g), then press **PT**.

The Net weight will be displayed.

When the weight is removed from the pan, the negative weight displayed is the Pre-set Tare value.

Weight g	Piece Weight g/pc	Count pcs
250.0	0.	0.
0.0	PrEtA	-----
200.0	PrEtA	-----
50.0	0.	0.
-200.0	0.	-----

NOTE: To clear the Tare or Pre-set Tare value, press **TARE** with the pan empty.

4.4 Zero Operation

Center of Zero is indicated by the **→0←** annunciator.

Press **ZERO** to zero the weight display. "CEnter" will be displayed momentarily before the display is zeroed.

Weight g	Piece Weight g/pc	Count pcs
-----	CEnter	-----
0.0	0.	0.

4.5 Sampling, Calculating Average Piece Weight (APW)

Place the desired sample onto the weighing pan (or into a tared container) (ex. 3000g).

Press **SAMPLE**. "SAmP" will be displayed momentarily before the calculated APW is confirmed (based on the last sample size entered or ex-factory default 10 if used for the first time). Or, enter a new sample size (ex. 50) via the numeric keypad before pressing **SAMPLE**.

Weight g	Piece Weight g/pc	Count pcs
3000.0	0.	0.
3000.0	SAmP	-----
3000.0	300.000	10.
3000.0	50.	60.
3000.0	SAmP	-----
3000.0	60.0000	50.

NOTES:

- The larger the sample size, the more accurate the APW.
- The sample size entered is retained even after the unit is turned off.
- Unless stored into memory (refer to *Sec.4.7*), Piece Weight values are not retained when the unit is turned off.

4.6 Entering a Known Piece Weight

Enter the value of a known piece weight via the numeric keypad (ex. 40g/pc.), then press **APW** (with a weight on the pan, the piece count is automatically calculated and displayed).

Weight g	Piece Weight g/pc	Count pcs
0.0	40.	0.
0.0	40.	0.

NOTE:

- To clear the Piece Weight value, press **C**.
- "Wt. Lo" annunciator will turn on if the total sample weight is less than 10 display divisions. Add more samples for a more accurate or stable reading.
- "APW Lo" annunciator will turn on if the APW value is less than 1/10th display divisions. Increase the piece weight value for more accurate results.

4.7 Storing Piece Weight into Memory

There are 10 memory locations (0 to 9 numeric keys) available to store APW values.

After determining the piece weight (refer to *Sec. 4.5 or 4.6*), long-press **APW** for approx. 2 seconds. "StorE" will flash on the display.

Press any one of the numeric keys to store the piece weight data in this selected location.

Weight g	Piece Weight g/pc	Count pcs
0.0	40.	0.
0.0	StorE	0.
0.0	40.0	0.

NOTE: Stored APW values are retained when the unit is turned off.

4.8 Recalling Piece Weight from Memory

Press the numeric key (ex. location 5) with the stored piece weight data (ex. 40 g/pc), then press **APW** two times. The stored data will be uploaded and displayed.

Weight g	Piece Weight g/pc	Count pcs
0.0	0.	0.
0.0	5.	0.
Memory Location		
0.0	40.000	0.

4.9 Accumulation: Weight and Quantity

Accumulation is indicated by the Σ^+ annunciator.

Place the item to be weighed/counted on the pan (ex. 300g with APW of 60g). Press **M+**. "Add", then the accumulation event is displayed momentarily before reverting to normal weighing mode.

NOTE: Weight display must return to zero before the next accumulation can register.

Weight g	Piece Weight g/pc	Count pcs
300.0	60.0000	5.
-----	Add	-----
300.0	Σ^+	5.
Total Accumulated Weight	Total Accumulation Times	Total Accumulated Count
300.0	60.0000	5.

To recall Total Accumulation data, press **M+** with no weight on the pan. The data is displayed momentarily before reverting to normal weighing mode.

Weight g	Piece Weight g/pc	Count pcs
1500.0	Σ^+	25.
Total Accumulated Weight	Total Accumulation Times	Total Accumulated Count
1500.0	60.0000	25.

To clear the Total Accumulation data, press **C** while the data is displayed.

NOTE: Accumulation data is not retained when the unit is turned off.

5 SCALE SETTINGS

- ☑ Long-press **TARE** to enter into the user-selectable scale settings (Setup mode).
- ☑ In Setup mode:
 - o Press **Sample** to step through available settings
 - o Press **Tare** to accept the displayed setting and proceed to the next Setup parameter
- ☑ Press **C** at any time to exit from the Setup mode.
- ☑ Re-start the scale after changing settings in the Setup mode

The following parameters are available:

5.1 Auto-Off

Sets the period of inactivity before the scale automatically turns off. The following settings are available: 0 = Off, 2, 5, 8 (minutes)

Weight g	Piece Weight g/pc	Count pcs
0.	A.OFF	-----
Default Setting	Auto-Off	Internal Count (disregard)

5.2 Zero Tracking Range

Sets the range in which the zero reading is maintained. The following settings are available: 0 = Off, 1 = 0.5d, 2 = 1d, 3 = 2d, 4 = 3d (d = scale division)

Weight g	Piece Weight g/pc	Count pcs
2.	Zero Tracking Range	-----
Default Setting	Zero Tracking Range	Internal Count (disregard)

5.3 Zero Display Range

Sets the range in which the Zero indication turns on. The following settings are available: 0 = Off, 1 = 0.5d, 2 = 1d, 3 = 2d, 4 = 3d (d = scale division)

Weight g	Piece Weight g/pc	Count pcs
3.	Zero Display Range	-----
Default Setting	Zero Display Range	Internal Count (disregard)

5.4 Filtering

Sets the level in which the Stable indication turns on; the higher the setting, the faster stabilization time. The following settings are available: 0, 1, 2, 3, 4, 5 (level)

Weight g	Piece Weight g/pc	Count pcs
4.	Filtering Level	-----
Default Setting	Filtering Level	Internal Count (disregard)

5.5 Zero Return Range

Sets the level in which the zero point is stable; the higher the setting, the more stable.

The following settings are available: 0, 1, 2, 3, 4, 5 (level)

Weight g 0.	Piece Weight g/pc 0.12E	Count pcs -----
Default Setting	Zero Return Range	Internal Count (disregard)

5.6 Backlight

Sets the activation mode of the backlight.

The following settings are available:
0 = Auto-on with items greater than 9d placed on the pan or any key is pressed; turns off after 5 seconds of inactivity.

1 = Manual; press the decimal point key [.] to switch the backlight on or off.

Weight g 0.	Piece Weight g/pc 0.1	Count pcs -----
Default Setting	Backlight	Internal Count (disregard)

5.7 Unit Selection

Sets the active weighing unit.

The following settings are available:
0 = Grams (g), 1 = Pounds (lb)

Weight g 0.	Piece Weight g/pc 0.12	Count pcs -----
Default Setting	Weighing Unit	Internal Count (disregard)

5.8 APW Re-computing

Sets the APW re-computing mode. Optimizes piece weight accuracy by automatically re-computing the existing APW as further pieces (less than the original quantity on the pan) are added (a beep will sound in this event).

The following settings are available:
0 = Off, 1 = On

Weight g 0.	Piece Weight g/pc 0.12	Count pcs -----
Default Setting	APW Re-averaging	Internal Count (disregard)

6. CALIBRATION

For best results, calibrate the scale at regular intervals. Temperature changes, geographic gravity variations, altitude changes and abuse are few reasons why a scale may need recalibration.

When the scale is ideally positioned for operation, enter calibration and proceed as follows:

Long-press **Zero** to initiate calibration (do not release key-press until "CAL" is displayed).

The required calibration weight is displayed (ex. 3000g for a 3kg model). At this time, a different calibration weight value can be entered via the numeric keypad.

Weight g	Piece Weight g/pc	Count pcs
0.	3000.0	CAL
Actual calibration weight	Required calibration value	Procedure

Place the corresponding calibration weight on the pan. The display flashes until the actual weight is registered and the calibration process ends (the scale momentarily beeps before exiting to normal weighing mode).

3000.0	3000.0	CAL
3000.0	3000.0	CAL
3000.0	0.	0.

NOTE: Press **Zero** at any time to abort during the calibration process.

7. TROUBLESHOOTING

The following table lists common problems, possible causes and remedies. If the problem persists, contact Ohaus or your authorized Ohaus dealer.

Symptom	Possible Causes	Remedy
Scale will not turn on.	AC power not connected. Battery discharged.	Connect scale to power. Connect scale to power and charge battery.
Battery fails to charge fully.	Battery is defective or past its useful life.	Have the battery replaced by an authorized Ohaus service dealer.
Weight reading does not stabilize.	Unstable environment. Interference under pan.	Ensure a stable environment. Ensure that the weighing pan is unobstructed and free to move.
Scale does not display accurately.	Improper calibration.	Calibrate the scale using proper calibration weights.
E1, E2, E3 displayed	The pan is placed incorrectly. Zero limit exceeded during power up.	Reposition the pan correctly. Ensure the pan is empty before switching the scale on.
--OL-- displayed	Load exceeds scale capacity.	Reduce the load on the pan.

8. TECHNICAL DATA

Model	EC3	EC6	EC15	EC30
Capacity x Readability	3000 g x 0.1 g 6 lb x 0.0002 lb	6000 g x 0.2 g 15 lb x 0.0005 lb	15000 g x 0.5 g 30 lb x 0.001 lb	30000 g x 1 g 60 lb x 0.002 lb
Maximum Displayed Resolution	1:30000	1:30000	1:30000	1:30000
Min Recommended Sample Weight	1 g / 0.002 lb	2 g / 0.005 lb	5 g / 0.01	10 g / 0.02 lb
Min Recommended APW	0.01 g / 0.00002 lb	0.02 g / 0.00005 lb	0.05 g / 0.0001 lb	0.1 g / 0.0002 lb
Construction	Stainless steel pan, plastic housing			
Weighing Units	g, lb			
Application Modes	Weighing, Counting, Accumulation			
Display	3-Window, 19 mm / 0.75" High, 6-digit, 7-segment backlit LCD display			
Display Indicators	Stability, Center of Zero, Tare, Low Sample Weight, Low APW, Accumulation, Battery status			
Hi-Lo Check Indicators	Display with Alert beeper			
Memories	10 locations for APW			
Keyboard	7 function, 11 numeric x Membrane switch: Tare, Sample, APW, Zero, Pre-set Tare, M+, Cancel			
Zero Range	4% of Full Scale Capacity			
Tare Range	Full Capacity by Subtraction (except EC15, up to 10kg only)			
Stabilization Time	≤ 2 seconds			
Operating Temperature	0° to 40°C			
Humidity Range	≤90% relative humidity, non-condensing			
Power	AC Adapter 12V DC / 800mA Internal rechargeable lead acid battery			
Battery Life	80 hours continuous use with 12 hour recharge time			
Calibration	Automatic external with kg mass			
Shipping Protection	Shipping screw to avoid damage to sensitive components			
Safe Overload Capacity	120% of capacity			
Pan Size	294 x 226 mm / 11.6 x 8.9 in.			
Scale Dimensions W x H x D	325 x 114 x 330.5 mm / 12.8 x 4.5 x 13 in.			
Shipping Dimensions W x H x D	440 x 160 x 360 mm / 17.3 x 6.3 x 14.2 in.			
Net Weight	4.2 kg / 9.2 lb			
Shipping Weight	5.3 kg / 11.7 lb			
Other Features	Auto-Zero Tracking, Filtering Level, Auto-Optimization of APW			

LIMITED WARRANTY

Ohaus products are warranted against defects in materials and workmanship from the date of delivery through the duration of the warranty period. During the warranty period, Ohaus will repair, or, at its option, replace any component(s) that proves to be defective at no charge, provided that the product is returned, freight prepaid, to Ohaus.

This warranty does not apply if the product has been damaged by accident or misuse, exposed to radioactive or corrosive materials, has foreign material penetrating to the inside of the product, or as a result of service or modification by other than Ohaus. In lieu of a properly returned warranty registration card, the warranty period shall begin on the date of shipment to the authorized dealer. No other express or implied warranty is given by Ohaus Corporation. Ohaus Corporation shall not be liable for any consequential damages.

As warranty legislation differs from state to state and country to country, please contact Ohaus or your local Ohaus dealer for further details.

Menu EC Series

A.OFF Sets the time of inactivity to auto turn off

- 0 — Off
- 2 — 2 Minutes to shutoff
- 5 — 5 Minutes to shut off
- 8 — 8 Minutes to shutoff

trAC Sets the range in which a small change in zero is cancelled out

- 0 — Off
- 1 — 0.5d
- 2 — 1d
- 3 — 2d
- 4 — 3d

ZERO Sets the range in which the zero indicator is on

- 0 — Off (Turns zero indicator off)
- 1 — 0.5d
- 2 — 1d
- 3 — 2d
- 4 — 3d

Filt Increases the number of times the displayed result is averaged

- 0 — Most filtering, Slowest Stabilization
- 1
- 2
- 3
- 4
- 5 — Least filtering, Fastest Stabilization

t.rATE Zero Return Range

- 0 — Least stable
- 1
- 2
- 3
- 4
- 5 — Most stable

Unit Weighing Units

- 0 — grams
- 1 — Pounds

bL Backlight control

- 0 — Automatic
- 1 — Manual

AU Average Piece weight recalculation

- 0 — Off
- 1 — On



Ohaus Corporation
19A Chapin Road
P.O. Box 2033
Pine Brook, NJ 07058, USA
Tel: (973) 377-9000
Fax: (973) 593-0359

With offices worldwide / Con oficinas en todo el mundo / Bvreaux dans le monde entire /
Weltweite Geshäftsstellen / Con uffici in tutto il mondo.
www.ohaus.com

© Ohaus Corporation 2005, all rights reserved / todas los derechos reservados / tous droits
reserves / alle rechte vorbehalten / tutti i diritti riservati.



P/N 80251009

Printed in China / Impreso en la China / Imprimé en Chine / Gedruckt in China /
Stampato in Cina